

STAMP guideline version 9.1 – January 26, 2022

Scandiatransplant Acceptable Mismatch Program (STAMP) and Local Acceptable Mismatch Program (LAMP)

STAMP	2
1. General STAMP guidelines	2
2. Finding the menu for entering STAMP-data	3
3. Selection of patients	5
3.1 Potential candidates	5
3.2 Good candidates?	5
3.3 Consult clinician	5
4. STAMP initial preparation	5
4.1 Registration of relevant HLA antibodies	5
4.2 Entering STAMP data	6
5. Quality check of STAMP data	7
6. Patients being prepared for STAMP	9
7. Patients ready to go on STAMP	9
8. Patients for evaluation	10
9. Communication during evaluation	11
10. Patients on STAMP	11
11. Quality control of antibody screening	11
12. Patients temporary off STAMP	13
13. Patients permanent off STAMP	14
14. STAMP reports	15
14.1 Patient STAMP details	15
14.2 Reports	16
LAMP	18
15. Introduction	18
16. Menus for entering LAMP-data and LAMP pre transplantation information	18
17. Patients ready to go on LAMP	18
18. Kidney search result LAMP	19
STAMP & LAMP	20
19. Calculated combined PRA and transplantability	20
19.1 Calculated combined PRA	20
19.2 Estimated transplantability score	21
19.3 Transplantability score	21
19.3 Normal match	22

STAMP

1. General STAMP guidelines

Purpose

To increase the likelihood of offering a suitable kidney graft to broadly sensitized recipients, thus reducing their time on the waiting list.

Acceptance criteria

1. Transplantability score (TS) ABO identical $\leq 2\%$ and ABO compatible $\leq 3\%$
2. The last tested sample drawn less than 3 months before acceptance

Recipient HLA typing

Recipient HLA-antigens must be assigned at split level by molecular (and serology) typing.

Recipient acceptable HLA-antigens

Definition of acceptable HLA-mismatches is performed by laboratory at recipient center.

Acceptable mismatches may be HLA-A, -B, -C, -DRB1, -DRB3/4/5, -DQA1, -DQB1, -DPA1, -DPB1 antigens.

Acceptable mismatches may include repeated mismatches from previous transplantations, but should mainly reflect the current immunization and not historical antibodies.

Definition of acceptable mismatches may be based on CDC and/or solid phase assays.

Wait listing and matching

Recipients own antigens and the defined acceptable mismatches are treated similarly.

Recipients in the program must be regularly screened at least every 3 months, antibody specificities must be re-evaluated at least once a year.

Once accepted, patients will stay included even if sensitization decreases.

For each donor search, a specific search among STAMP-recipients based on split level HLA, is performed. Exchange obligation is marked when the donor only has HLA-A, -B, -C, -DRB1, -DRB3/4/5, -DQA1, -DQB1, -DPA1, -DPB1 antigens specified as recipient's own or acceptable.

If there is more than one STAMP candidate when doing the search for kidney exchange obligations the recipients must be prioritised in the following order

1. Lowest TS, ABO compatible
2. ABO identical recipients
3. Same country as donor
4. Longest waiting time

The search result list is sorted by a calculated AMP-score, which is a weight score based on these priorities.

Re-evaluation by the steering committee

A STAMP patient not transplanted with a shipped kidney because of a positive cross-match must be temporarily withdrawn from STAMP, re-evaluated and eventually re-admitted.

Event reporting

Exchanged organ may be used for other local recipient if the indicated STAMP patient for any reason cannot be transplanted, reason must be recorded.

Recipient center must give detailed follow-up information on performed transplantations.

Steering committee:

The STAMP steering committee (SC) is a scientific subgroup of the Tissue Typers Group, which is an expert advising committee for the Nordic Kidney Group.

SC shall be composed of one tissue typer from each of the countries within Scandiatransplant together with a clinical representative from each country represented in the Nordic Kidney Group.

Proposals of STAMP candidates from individual centers must be evaluated and accepted by two of the tissue typers in the SC from which the candidate does not originate from. The evaluation by the SC is performed within four weeks from the date that recipient center has activated the patient for evaluation.

SC must keep updated on all effects of the program, including:

- Number of exchanged organs.
- Changes in waiting time for STAMP recipients and for other waiting patients.
- Changed reactivity in individual waiting recipients
- Positive cross matches at donor center.
- Fate of performed transplants.

SC must give yearly status reports to Scandiatransplant.

At the annual Scandiatransplant Tissue Typer Group meetings, individual cases on patients who have been waiting for years on the STAMP list can be brought up for discussion.

2. Finding the menu for entering STAMP-data

Enter patient identification (Scandia no. / date of birth) and press search

Click on the relevant patient on the search result list

Click on the active kidney waiting list entry (no information in the 'Termination' column):

Recipient information Info Back Save Reset Print

Scandia Number: 19 Nationality: S: Sweden Sex: M: Male

Date of Birth: Person Number:

Surname: First Name:

Transplantation History: (1)KI 07-JUN-2018; LI; PA; IT; HE; LU; CO;

Recipient Status: ALIVE; on STAMP

Waiting list status: N: Notified Waiting list type: KI: Kidney Urgency: T: Transplantable Treatm. center:

First regist.: 30-Jun-2017 Latest regist.: 18-Nov-2020

Basic info Clinical data Address/Phone HLA Typing Antibody Screen Test Fusion Acceptable Antibodies Previous Mismatches Death

ABO Blood Group: 0 Rhesus D: POS

Transplant center: ST: Stockholm Department: 89: Tx.Surg Kidney/Pancreas/Liver

Notes on Patient:

Waiting List

Add new

Waiting List	Date of entry	Termination
KI: Kidney	24-Jun-2019	
KI: Kidney	30-Jun-2017	Transplantation - deceased donor <- Donor: 94565, Tx-date: 07-JUN-18

Any patient with a kidney treatment record will have the STAMP tabs available.

Waiting list information Info Back Save Reset Print STAMP Print LAMP

Generic data

Scandia Number: 203 Surname: Surname:

Waiting list type: KI: Kidney Date of entry: 16-Jan-2020

Urgency: T: Transplantable

Future Withdrawn from: Future Withdrawn to:

Date of first urgency: 16-Jan-2020 Date of last urgency: 16-Jan-2020

Transplant center: OS: Oslo Treatment/dialysis center:

Immunization: HI: Highly immunized Date of last change of Immunization: 29-Jan-2021

STAMP Sign Up: Y: Yes STAMP Status: A: Active

Specific data Infection LAMP LAMP QC STAMP STAMP log STAMP Aux STAMP QC Urgency History Termination

Determination Method: LUMI

Date of acceptance: 04-Feb-2021 Status: A: Active Sign up: Y: Yes

Acceptable mismatches

HLA-A: 11,30,31,34,43,74

HLA-B: 35,39,46,48,54,55,56,67,71,72,73,75,78,81

HLA-Cw: 1,2,3,4,5,6,8,10,12,14,15,16,17,18

HLA-DR: 1,10,16,103

HLA-DQ: 4,5,7,9

HLA-DP: 0501,1101,1301,1501,1901,2301

HLA-DRB3/4/5: 5*02

HLA-DQA: 02,04,05,06

HLA-DPA: 03,04

3. Selection of patients

3.1 Potential candidates

Potential candidates can be found by entering the list from the menu entrance 'Quality Control' -> 'Estimated TS \leq 2% with no STAMP record'. This list contains patients that are highly sensitized and have antibody specificities recorded in the system.

3.2 Good candidates?

Evaluate if the potential STAMP eligible patient have difficulties in getting a kidney from a local donor.

- Good candidates usually have a reason for sensitization (previous transplants, pregnancies, or blood transfusions).
- Good candidates often have both CDC and solid phase reactivity.
- Good candidates usually have high-level reactivity in antibody testing.
- Good candidates occasionally have a history of positive cross matches.

3.3 Consult clinician

Consult clinician about the need for STAMP or any other type of prioritizing. Consider both STAMP and LAMP and decide what is best for the particular patient.

4. STAMP initial preparation

4.1 Registration of relevant HLA antibodies

A summary of all registered antibodies can be viewed in the 'STAMP Aux' tab.

Generic data

Scandia Number: 205; Surname: Surname: ...
Waiting list type: KI: Kidney Date of entry: 20-Nov-2020
Urgency: T: Transplantable
Future Withdrawn from: Future Withdrawn to:
Date of first urgency: 20-Nov-2020 Date of last urgency: 20-Nov-2020
Transplant center: OD: Odense Treatment/dialysis center:
Immunization: LI: Low immunized Date of last change of Immunization: 02-Nov-2020
STAMP Sign Up: Y: Yes STAMP Status: A: Active

Specific data Infection LAMP LAMP QC STAMP STAMP log STAMP Aux STAMP QC Urgency History Termination

Antibody Summary: A:1,3,11,24,25,26,30,31,33,34,36,43,66,68,69,74,80 B:44,45,73,76 Cw:4,6,7,18 DQ:(6) DR:1,103,9,10,15,16 DRB3/4/5:5

Own HLA: A*2,32;B*61,51;C*2,14;Bw*w4,w6;DRB1*11,13;DPB1*0301,0402;DQB1*7,6;DRB345*3*01,3*02;DQA1*0103,0505;DPA1*01

Calculated Combined PRA: 98 %

Previous Mismatches

Series	Antigene	Acceptable mismatch	Tx. registration in SCTP
--------	----------	---------------------	--------------------------

Antibody Screen Test

Date of sample	PRA Class I	Method Class I	PRA Class II	Method Class II	Identified Antibodies
1 02-Nov-2020	4	CDC	4	CDC	

Antibodies with () are no longer clinical relevant, these can be given by selecting them through the 'Acceptable Antibodies' tab on the recipient.

- Include all antibodies that are positive according to local rules (e.g. all with Luminex MFI level > 1000)
- If allele specific antibodies are detected, consider adding them at serological level if the allele is not extremely rare. Remember that you do not know ethnical background of potential donor beforehand!

4.2 Entering STAMP data

4.2.1 Determination method

Click on the field 'Determination method' and select one to many from the list

4.2.2. Acceptable mismatches

Acceptable mismatches are selected from the lists or entered one by one.

The screenshot shows the STAMP data entry interface. At the top, there are tabs for 'Specific data', 'Infection', 'LAMP', 'LAMP QC', 'STAMP', 'STAMP log', 'STAMP Aux', 'STAMP QC', 'Urgency History', and 'Termination'. The 'STAMP' tab is selected. Below the tabs, there are fields for 'Determination Method' (set to 'CDC,LUMI'), 'Date of acceptance' (set to '17-Mar-2020'), 'Status' (set to 'A: Active'), and 'Sign up' (set to 'Y: Yes'). The 'Acceptable mismatches' section is highlighted, showing a list of HLA antigens with their corresponding mismatch counts. The list includes HLA-A (30,31,32,33,69,74), HLA-B (Select all...), HLA-Cw (1), HLA-DR (9), and HLA-DQ (11). The HLA-A field is expanded, showing a list of antigens with their mismatch counts: 2,77,78.

Deselect by clicking on the antigen specificity again

'Select all' will select all antigens on the list as acceptable mismatches

'Select calculated' will select all antigens that the recipient has no HLA antibodies against.

How to select antigens to be listed as acceptable mismatches (AMM)

- All antigens that the patient has no antibodies against could usually be added to the AMM list. These may also include possible previous mismatches.
 - If you add DR17 remember to **add** DR3 also.
 - If you add both Cw9 and Cw10 **add** Cw3 also.
 - Other broad serological level antigens may be added if all splits are on the AMM list, but usually are not necessary since laboratories type these at split level.
- Own known antigens cannot be added to the AMM list. Add most likely own (according to haplotype analysis) antigens to the AMM list if these are not typed and reported.
- If you have an allele specific antibody against patient own antigen (different allele) it is usually better to remove that antigen-with an explanation-from the patient typing

4.2.3 Date of acceptance

Date of acceptance is automatically inserted when the recipient has been accepted and 'Sign up' is changed to 'Yes'.

4.2.4 Status

When you are preparing the patient set the status to Inactive/calculation

Specific data	Infection	LAMP	LAMP QC	STAMP	STAMP log	STAMP Aux	STAMP QC	Urgency History	Termination
Determination Method: CDC,LUMI									
Date of acceptance: 17-Mar-2020		Status: I: Inactive		Sign up: N: No					
Acceptable n									
HLA-A: 30,31,32,33,69,74		C: Calculation							
HLA-B: 5,7,12,16,17,21,22,27,35,38,41,44,45,47,48,49,50,51,52,5		I: Inactive							
HLA-Cw: 4,5,15,17,18									
HLA-DR: 10,103									

4.2.5 Comments

Write all relevant information in the comments field. At least the following information should be added:

- List of all detected allele specific antibodies that are not added at serological level to the antibody list.
- List of all antigens that are not included to the antibody or AMM list for any reason.
- All other relevant information that SC should know

HLA-DRB3/4/5: 4*01,5*01	
HLA-DQA:	
HLA-DPA: 02,03,04	
Comments: Previous mismatches DR9 and B40 (thus B60 is removed).	

TIP!

You can always start entering data on the patient– leave the patient – with status inactive and return to enter more data later.

5. Quality check of STAMP data

When all data have been entered on the patient a quality check must be performed. Go to the tab 'STAMP QC'

Specific data	Infection	LAMP	LAMP QC	STAMP	STAMP log	STAMP Aux	STAMP QC	Urgency History	Termination
Quality control - STAMP preconditions									
TS, ABO identical <= 2%:		Yes (1.65%)							
TS, ABO compatible <= 3%:		No (5.5%)							
HI PRA >= 80% at present:		No (I Immunized)							
Most recent PRA < 3 months:		No (22-JUL-2021 5 months 28 days)							
Correct HLA typing resolution:		Yes (A 3,25; B 18,55; Cw 9,12; DR 4,13; DQ 6,8; DPB1 *0401,1401; DQA1 *0102,0301; DPA1 *0103,0201; DRB *3*0301,4*0103)							
Acc. mm. splits:		Yes (All acc. mismatches are splits)							
Id. antib. splits:		Yes (All identified antibodies are splits)							
No identif. AB in Acc. mm.:		Yes (No identified AB in AM)							
No identif. AB in own HLA:		Yes (No identified AB in own HLA)							
Consistent Sero/Geno HLA:		Yes (Consistent Sero/Geno HLA)							
All HLA checked:		Yes (All HLA checked)							

The STAMP QC will give you an indication of the quality of the registered data.

Green colour = quality check passed

Red colour = quality check did NOT pass, mandatory according to the STAMP guidelines, please check and/or add explanation to comment field

Orange colour = quality check NOT passed, please check and/or add explanation to comment field

The STAMP check is a quality control and is meant as a help, it does not inflict with the activation of patients to STAMP. If you have an explanation of why criteria are not fulfilled, please enter it in the comment field.

The quality check and calculations are done on the following variables:

TS, ABO identical \leq 2% (obligatory to fulfil)

Checks if the current ABO identical transplantability score is \leq 2%

TS, ABO compatible \leq 3% (obligatory to fulfil)

Checks if the current ABO compatible transplantability score is \leq 3%

HI PRA \geq 80% at present

Defines if the patient is highly immunized (PRA \geq 80%) in last registered antibody screen test

Most recent PRA < 3 months (obligatory to fulfil)

Checks if the last registered antibody screen test is done on serum drawn within the last 3 months

A, B, C, DR, DQ splits

A check is done whether the recipient HLA-antigens are assigned at split level. A '*' in front of an allele indicates that the assigned HLA type contains a broad serological type. A '!' in front of an allele indicates that there is a broad genomic type.

Result of the QC check may be No, if so check carefully that the reason for No is something you have intended.

Acc. mm. splits

Checks if all acceptable mismatches are registered as splits

Result of the QC check May be No, if so check carefully that the reason for No is something you have intended.

Id. antib. splits

Checks if all identified antibodies are registered as splits

Result of the QC check may be No, if so check carefully that the reason for No is something you have intended.

No identif. AB in Acc. mm.

Compares one to one if any identified antibodies by mistake are given as acceptable mismatches.

Consistent Sero/Geno HLA

Compares the patient's own serological and genomic HLA as it is registered in the database

All HLA checked

Listing all antigens not given as own HLA antigens, acceptable mismatches or identified antibodies.

Result of the QC Check may be No. If so, check carefully that you have mentioned not to include some antigens and that you have explained reasons not to include some antigens (for instance if antigens are left out due to linkage or if these are considered as “grey zone”).

6. Patients being prepared for STAMP

Finding the patients being prepared for STAMP, enter the menu ‘All recipients’ and register the search parameters below (Status should be either Inactive or calculation)

All Recipients Search Add new Print Statistics Reset

[Enter search parameters]

Scandia Number: Nationality:

Person Number: Sex: Age ≥ < Age at notif. ≥ <

Surname: First Name:

Transplant Center: Recip.AB0: Donor AB0: Wait.time ≥ < months

Waiting list status: Waiting List type: Urgency: Local Urgency:

STAMP Extra

Sign up: N: No Positive infection:

Status: Kidney Prefs.:

A: Active
C: Calculation
I: Inactive
L: Local programme

Scandi... Natic... Recip.... Height Weight Waitin... Waitin... Urgency

Page 1 of 4 Order by: Scandia Number Recip.AB0

Displaying 1 - 25 of 92

7. Patients ready to go on STAMP

When you have done the quality check and you believe that sufficient data has been entered you have to change "Status" from I/C to A and save data.

', 'Status: I: Inactive', and 'Sign up: N: No'. Below this, there are two rows of HLA data: HLA-A: 3,11,23,24,25,26,29,30,31,32,33,34,36,43,66,69,74,80 and HLA-B: 18,27,39,41,45,47,54,59,60,61,64,65,73,82. A dropdown menu for Status is open, showing options: A: Active, C: Calculation, and I: Inactive."/>

Specific data Infection LAMP LAMP QC **STAMP** STAMP log STAMP Aux STAMP QC Urgency History Termination

Determination Method: LUMI

Date of acceptance: Status: I: Inactive Sign up: N: No

Acceptable n

HLA-A: 3,11,23,24,25,26,29,30,31,32,33,34,36,43,66,69,74,80

HLA-B: 18,27,39,41,45,47,54,59,60,61,64,65,73,82

A: Active
C: Calculation
I: Inactive

An e-mail will now be sent to the committee and they will go through the patient to see if it is valid for the program. The results of the STAMP quality check will automatically be included in the email message.

Example of part of an email message

Scand 181 updated 2/4/2021 7:48:56 AM by Not signed up, changed status to Active

Serological HLA: A2,11;B13,53;Cw4,6;DR7,13;DQ2,6;Bw4

Genomic HLA: A*0201,1101;B*1302,5301;C*0401,0602;DRB1*0701,1302;DPB1*0401,1701;DQB1*

Identif. Antib.: A:1,23,24,(80)

B:(7),(8),(18),(35),(39),(41),(42),44,45,(46),(48),(49),(50),(54),(55),(56),(60),(61),(62),
(64),(65),(67),(71),(72),(75),76,(78),(81),82

Cw:(1),(8),(10)

DQ:4,7,8,9

DQA:03,04,05

DR:1,4,(14),15,(18)

Calc. comb. PRA: 98

Acc. Mism.: A3,25,26,29,30,31,32,33,34,36,43,66,68,69,74,80

B7,8,18,27,35,37,38,39,41,42,46,47,48,49,50,51,52,54,55,56,57,58,59,60,61,62,63,64,65,67,71,72,
Cw1,2,5,7,8,9,10,12,14,15,16,17,18

DP0101,0201,0301,0402,0501,0601,0901,1001,1101,1301,1401,1501,1801,1901,2001,2301,2801

DPA03,04

DQ5

DR103,8,9,10,11,12,14,16,17,18


DRB3*01,3*02,5*01,5*02

TS <= 2%: Yes (.75%)

PRA < 3 months: Yes (18-NOV-2020 2 months 17 days)

8. Patients for evaluation

STAMP patients ready for evaluation is found by entering the 'Quality Control' menu and selecting 'Candidates for evaluation':

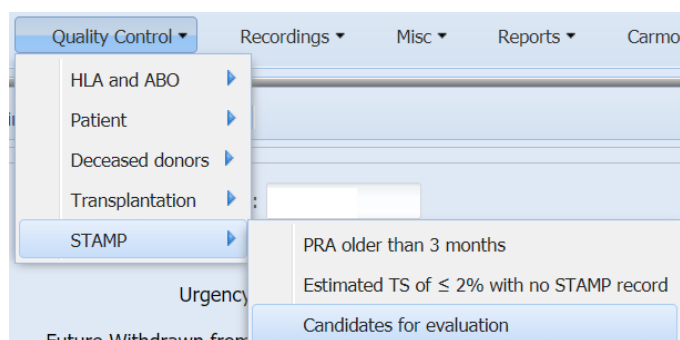

9. Communication during evaluation

Approval/disapproval and communication about each specific patient must be done on the related waiting list record in the 'STAMP log' tab. To add information in the table, click below the 'Comments' column header.

Specific data	Infection	LAMP	LAMP QC	STAMP	STAMP log	STAMP Aux	STAMP QC	Urgency History	Termination
STAMP event history									
	STAMP Status	STAMP SignUp	Date of change	User	Cause of withdr.				
1	A: Active	Y: Yes	17-Mar-2020						
2	A: Active	N: No	21-Feb-2020						
3	C: Calculation	N: No	14-Jan-2019						
STAMP evaluation status									
	Approved	Date of change	User	Comments					
➡		08-Feb-2021		Click here to add new evaluation/comment					
➡	Y: Yes	17-Mar-2020		I guess that the PRA values listed are CDC, whereas the antibodies are by Luminex to account for the T...					
➡	Y: Yes	26-Feb-2020		ok for me but later I think some DPA,DQA should be added as acceptable.					

Each time information is added in the STAMP evaluation table an e-mail with updated information will be sent to the STAMP committee and persons working on the patient record.

10. Patients on STAMP

In the menu 'All recipients' enter the search parameters below and you will find all patients on STAMP. If you only wish to see patients belonging to a specific tx. center you can add it is as a search parameter.

All Recipients Search Add new Print Statistics Reset

[Enter search parameters]

Scandia Number:

Nationality:

Person Number:

Sex:

Age ≥ <

Age at notif. ≥ <

Surname:

First Name:

Transplant Center:

Recip.AB0:

Donor AB0:

Wait.time ≥ < months

Waiting list status:

Waiting List type:

Urgency:

Local Urgency:

STAMP

Sign up: Y: Yes
Status: A: Active


Extra

Positive infection:
Kidney Prefs.:

	Scandi...	Nation...	Person Number	Age	Surname	First Name	Transp...	Recip....	Height	Weight	Waitin...	Waitin...	Urgency
Page	1	of 4	Order by:	Scandia Number ▼	Recip.AB0 ▼	Displaying 1 - 25 of 92							

11. Quality control of antibody screening

Patients on STAMP must be HLA antibody screen tested at least every 3 months. To ensure that all active STAMP patients complies with this rule go to the menu 'Quality Control' -> 'STAMP - PRA older than 3 months'.

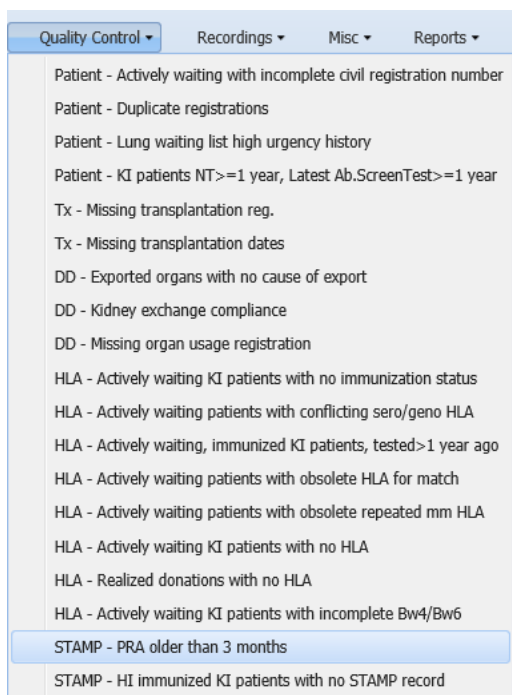

By entering this menu, you get a display of patients missing the regular antibody screen test. To the right is a count of months and days since last registered screen test.

- STAMP listed patients must be screened at least every 3 months, and antibody specificities must be re-evaluated at least yearly. However, it is obligatory to perform the AMM list re-evaluation immediately when you notice significant changes in patient's immunization status, although the patient may have been previously evaluated less than a year ago.
- Add all new antibodies into the detected antibodies list and remove the same antigens from the AMM list. This does not necessitate steering group re-evaluation.
 - If the new antibody is allele specific, add it to antibody list at serological level if it is not extremely rare and remove the antigen from the AMM list. Information of very rare new allele specific antibody could be only added to the comments field without changing the AMM list.
- If your patient's immunization status has improved, you may consider register previously detected antibodies as allowable antibodies and adding them into the AMM list.

12. Patients temporary off STAMP

After acceptance to STAMP, the center responsible for the patient, has the possibility to remove the patient temporary from the program (for instance after a positive X-match). If you want to do so, you have to change "Status" from A = Active to I = Inactive.

Determination Method: LUMI

Acceptable mismatches

HLA-A: 26

HLA-B: 18,65

HLA-Cw: 1,4,5,6,12,14,15,16,17,18

HLA-DR: 1,103,10,3,4,7,8,9,12,13,14,15,16,18

HLA-DQ: 4,5,6,8,9

Date of acceptance: 20-Jul-2015

Status: I: Inactive

Sign up: Y: Yes

Comments:

First Registr.: 20-Jul-2015

Last Change.: 22-Sep-2016

Calculated transplantability

STAMP match: 0.40 %

Normal match: 0.20 %

Date of Last Calc: 29-Dec-2015

Cause of withdr.: ADDABS: Further antibody specification required
ADDHLA: Further HLA typing required
OT: Other, not specified cause
PXMTCH: Positive crossmatch: HLA typing and antibody specification required

STAMP Status	N: No	Date	Cause of withdr.
1 A: Active			
2 A: Active	N: No	16-Sep-2016	NAPEROS
3 I: Local programme	N: No	20-Jul-2015	OPS\$NAPEROS
4 I: Inactive	N: No	20-Jul-2015	OPS\$NAPEROS

Please select cause of temporary withdrawal.

Note

The patient will of cause still be searchable in Kidney-search only the STAMP exchange obligation will be suppressed.

To find "Patients temporarily off STAMP"

All Recipients

Search Add new Print Statistics Reset

[Enter search parameters]

Scandia Number: Nationality: Sex: Age ≥ < Age at notif. ≥ <

Person Number: Surname: First Name: Wait.time ≥ < months

Transplant Center: Recip.ABO: Donor ABO: Urgency: Local Urgency:

Waiting list status: Waiting List type:

STAMP Sign up: Y: Yes Status: I: Inactive

Extra Positive infection: Kidney Prefs:

Scandi...	Nation...	Person Number	Age	Surname	First Name	Transp...	Recip....	Height	Weight	Waitin...	Waitin...	Urgency
No data to display												

Page 0 of 0 Order by: Scandia Number Recip.ABO

Perform thorough re-evaluation of the case and change the antibody/ the AMM list accordingly

Write the information of all changes and your opinion of the reason for positive cross match into comments field.
 Finally change the status from I = Inactive to A = Active and the patient will be re-evaluated by the steering group.

13. Patients permanent off STAMP

Patients no longer eligible for STAMP, must be permanently withdrawn from STAMP.

Specific data	Infection serology	STAMP/LAMP	STAMP Aux	STAMP QC	Urgency History	Termination															
Determination Method: LUMI																					
Acceptable mismatches																					
HLA-A: 26																					
HLA-B: 18,65																					
HLA-Cw: 1,4,5,6,12,14,15,16,17,18																					
HLA-DR: 1,103,10,3,4,7,8,9,12,13,14,15,16,18																					
HLA-DQ: 4,5,6,8,9																					
Date of acceptance: 20-Jul-2015		Status: A: Active		Sign up: Y: Yes																	
Comments:																					
First Registr.: 20-Jul-2015		Last Change.: 22-Sep-2016																			
Calculated transplantability																					
STAMP match: 0.40 %		Normal match: 0.20 %		Date of Last Calc: 29-Dec-2015																	
Cause of withdr.:		Permanent Withdrawal:																			
		EVNOCR: Reevaluated, does not meet STAMP criteria NOMMHL: HLA antibodies / acceptable mismatches cannot be provided NOPRA: PRA not provided according to rules NOTACC: Not accepted on STAMP OT: Other cause PRNOCR: In preparation, does not meet STAMP criteria XMATCH: Persistent positive cross match																			
<table border="1"> <thead> <tr> <th></th> <th>STAMP Status</th> <th>STAMP SignUp</th> </tr> </thead> <tbody> <tr> <td>1</td> <td>A: Active</td> <td>Y: Yes</td> </tr> <tr> <td>2</td> <td>A: Active</td> <td>N: No</td> </tr> <tr> <td>3</td> <td>L: Local programme</td> <td>N: No</td> </tr> <tr> <td>4</td> <td>I: Inactive</td> <td>N: No</td> </tr> </tbody> </table>								STAMP Status	STAMP SignUp	1	A: Active	Y: Yes	2	A: Active	N: No	3	L: Local programme	N: No	4	I: Inactive	N: No
	STAMP Status	STAMP SignUp																			
1	A: Active	Y: Yes																			
2	A: Active	N: No																			
3	L: Local programme	N: No																			
4	I: Inactive	N: No																			

Select cause from list of value and save data.

14. STAMP reports

14.1 Patient STAMP details

When you have a STAMP-patient (active/on hold/ withdrawn) on screen you can press the STAMP print button to display STAMP data on the screen.

Waiting list information

Back Save Reset **Print STAMP**

Generic data

Scandia Number: ----- Surname: -----

Waiting list type: KI: Kidney Date of entry: 23-Jan-2015

Urgency: T: TransplantableX Future Withdrawn from: ----- Future Withdrawn to: -----

Future Withdrawn from: ----- Date of first urgency: 23-Jan-2015 Date of last urgency: 07-Jun-2016

Transplant center: GO: Göteborg Treatment/dialysis center: -----

Immunization: HI: Highly immunized Date of last change of Immunization: 20-Apr-2016

STAMP Sign Up: Y: Yes STAMP Status: A: Active

Specific data Infection ecology STAMP/I AMB STAMP A/B STAMP C/D Urgency History Termination

A typical printout will look like this

SCANDIATRANSPLANT stamp_details
Report produced: 09-FEB-2021 11:09 requested by user: Page 1

| STAMP details |

Scandianumber: 2044
Person number:
Gender: F Female
Name:
Country: S Sweden
Tx-Center: GO
Dialysis/Treatment center: BQ MÅ-LNDAL, Dialysavd
Waiting list: KI Kidney
Date of entry on waiting list: 23-JUN-2020
Waiting list status: N Notified
Waiting for tx number: 1
Blood group: 0
Narrow HLA: A 2,29;B 63,51;Cw 14,15;DR 4,12;DQ 7,8;
Repeated mismatches:
Antibody Screen Test: 24-OCT-2020 I% 98 CDC, FLOW II% 6 CDC, FLOW
01-JUL-2020 I% 93 FLOW, LUMI II% 0 FLOW, LUMI
Identified antibodies: A:1,3,11,23,24,32,36,43,66,80 B:7,8,13,18,27,35,
37,38,39,41,42,44,45,47,48,49,50,54,55,56,59,60,
61,62,64,65,67,71,72,73,75, 76,77,78,81,82 Cw:2,
4 DR:11 DRB3/4/5:5*01
Date of entry on STAMP: 07-AUG-2020
Date of acceptance on STAMP: 13-NOV-2020
Signed up: Y Yes
STAMP status: A Active
Determination methods: LUMI
Acceptable mismatches: A25,26,30,31,33,34,68,69,74 B46,52,53,57,58 Cw1,
5,6,7,8,9,10,12,16,17,18 DP0101,0301,0402,0501,
0601,0901,1001,1101,1301,1401,1501,1701,1801,

1901,2001,2301,2801 DPA02,03,04 DQ2,4,5,6,9
DQA01,02,04,06 DR1,103,7,8,9,10,13,14,15,16,17,
18 DRB3*02,3*03,5*02

Comments:

STAMP events:

N:I:07-AUG-2020:xx,N:A:07-SEP-2020:xx,
Y:A:13-NOV-2020:xx

Most recent PRA < 3 months

HI PRA >= 80% at present

HI >= x2 > 3 months

A,B,Cw,DR,DQ splits

Acc. mm. splits

Id. antib. splits

No identif. AB in Acc. mm.

Consistent Sero/Geno HLA

All HLA checked

First registered:

Last changed:

No 24-OCT-2020 3 months 16 days

Yes HI Highly immunized

Yes samples over 19 months 4 days

Yes (All acc. mismatches are splits)

Yes All identified antibodies are splits

Yes No identified AB in AM



Yes Consistent Sero/Geno HLA

07-AUG-2020 xx


13-NOV-2020 xx

14.2 Reports

A variety of STAMP reports are available in Reports -> More..:

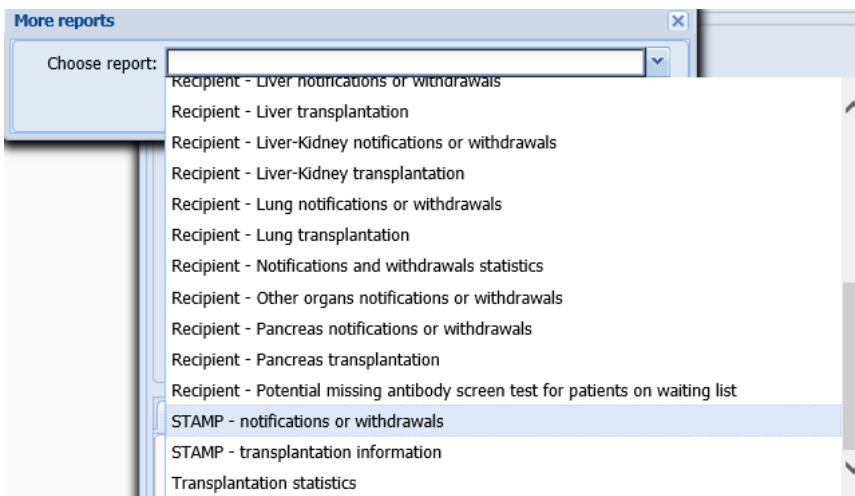

Selecting STAMP notifications or withdrawals

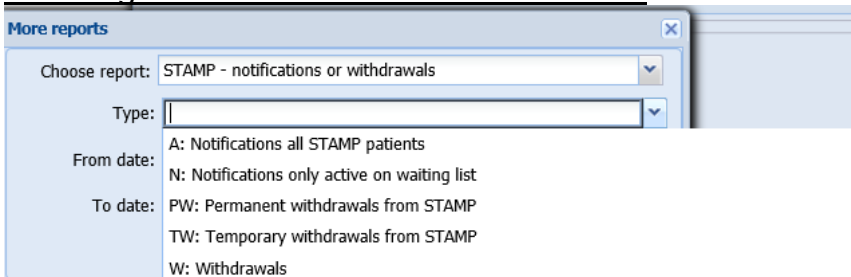

A: Notifications all STAMP patients

If you choose this report you will get all patients with a STAMP record. In other words, the report will contain patients that are: Preparing to go on STAMP, active/on hold on STAMP, transplanted, permanently withdrawn and dead.

N: Notifications only active on waiting list

Gives you patients with a STAMP record active/on hold in the specified period

PW: Permanent withdrawals from STAMP

This extraction contains patients permanent withdrawn from STAMP together with cause and date.


TW: Temporary withdrawals from STAMP

If you choose this report you will get a list of patients that have been temporary off STAMP along with cause and date.

W: Withdrawals

Consist of all patients with a STAMP record that have been permanent withdrawn from the main kidney waiting list.

Selecting STAMP notifications or withdrawals

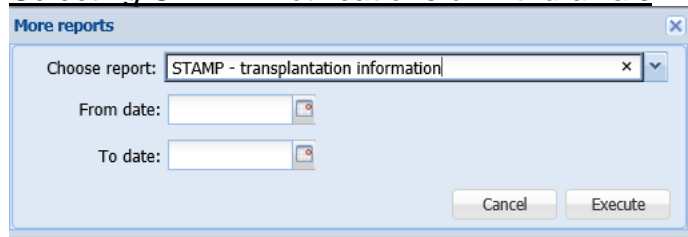

More reports

Choose report: STAMP - transplantation information x v

From date: [] []

To date: [] []

Cancel Execute

If you choose this report you will get a list of patients transplanted while they were signed up on STAMP waiting list.

It is possible to do the extraction for a specific period just enter starting and/or ending date.

LAMP

15. Introduction

Purpose

This program is a local version of STAMP. At recipient search the patients are matched the same way as STAMP patients, due to defined acceptable mismatches. The program does not result in any exchange obligations between centers.

Acceptance criteria

Each center defines the acceptance criteria themselves and there is no approval for inclusion to the program from the committee, patients can go directly on LAMP.

16. Menus for entering LAMP-data and LAMP pre transplantation information

To create a new LAMP-record search forward the recipient the same way as described for STAMP point 2.

To find patients with an existing LAMP record you can search on patient ID or you can use the 'Active on LAMP' search option:

The screenshot displays the LAMP search interface. At the top, there are tabs for 'All Recipients' and 'Info', and buttons for 'Search', 'Add new', 'Print', 'Statistics', and 'Reset'. Below these is a search form with the following fields:

- Scandia Number: [text input]
- Nationality: [dropdown menu]
- In STEP prg.: ☐
- Alive: ☐
- Person Number: [text input]
- Sex: [dropdown menu]
- Age ≥ [text input] < [text input]
- Age at notif. ≥ [text input] < [text input]
- Surname: [text input]
- First Name: [text input]
- Transplant Center: [dropdown menu]
- Recip.ABO: [dropdown menu]
- Donor ABO: [dropdown menu]
- Wait.time ≥ [text input] < [text input] months
- Waiting list status: [dropdown menu]
- Waiting List type: [dropdown menu]
- Urgency: [dropdown menu]
- Local Urgency: [dropdown menu]

Below the search form, there are two sections: 'AMP' and 'Extra'. The 'AMP' section includes:

- STAMP sign up: [dropdown menu]
- STAMP status: [dropdown menu]
- Active on LAMP: [dropdown menu]

The 'Extra' section includes:

- Positive infection: [dropdown menu]
- Kidney Prefs.: [dropdown menu]

At the bottom, there is a table with the following columns: Scandi..., Nation..., Person Number, Age, Surname, First Name, Transp..., Recip..., Height, Weight, Waitin..., Waitin..., and Urgency. The table is currently empty, and the status 'No data to display' is shown. The page number is 0 of 0, and the order by is Scandia Number.

17. Patients ready to go on LAMP

Enter LAMP information in the dedicated tab and select 'Yes' when you want to activate the patient on LAMP:

Waiting list information Info Back Save Reset Print STAMP Print LAMP

Generic data

Scandia Number: Surname:

Waiting list type: KI: Kidney Date of entry: 22-Oct-2020

Urgency: T: Transplantable Future Withdrawn from: Future Withdrawn to:

Date of first urgency: 22-Oct-2020 Date of last urgency: 22-Oct-2020

Transplant center: OS: Oslo Treatment/dialysis center: 02: Ullevål

Immunization: I: Immunized Date of last change of Immunization: 26-Dec-2020

STAMP Sign Up: N: No STAMP Status: I: Inactive

Specific data Infection LAMP LAMP QC STAMP STAMP log STAMP Aux STAMP QC Urgency History Termination

Active on LAMP: Y: Yes N: No

HLA-A Y: Yes

HLA-B: 7,13,27,35,38,41,44,45,47,48,49,50,52,53,55,56,57,60,61,62,63,67,71,72,73,76,77,82

HLA-Cw: 1,2,3,4,5,7,8,9,10,12,14,15,16,17

HLA-DR: 1,3,4,7,8,9,10,12,14,15,16,17,18,103

HLA-DQ: 2,4,5,8,9

HLA-DP: 0201,0301,0402,0501,0601,0901,1001,1101,1301,1401,1501,1701,1801,1901,2001,2301,2801

HLA-DRB3/4/5: 3*01,3*03,4*01,5*01,5*02

HLA-DQA: 02,03,04,06

HLA-DPA: 03,04

18. Kidney search result LAMP

In the kidney search result screen a LAMP match will appear as a priority 6 match and marked with a 'L' in the STAMP status column.

Search for suitable kidney recipient Search Print Reset

[Enter search parameters]

Donor: Donor number:

Recipient Center: OS Date of birth: 01-Jan-2010 AB0 Blood Group: A

Serologic HLA Genomic HLA

A: 1 26 B: 7 18 A: C: Bw4/Bw6: DRB1: DQB1:

Cw: 7 Bw4/Bw6: DRB1: DQB1:

DR: 13 DQ: 6

HLA-search: A1,26;B7,18;Cw7;DR13;DQ6 Calculated Bw: w6

No extra filters added ...

Pri...	Sc.No	Rec...	Surname	First Name	Age	Wa...	Tx...	Im...	AB0	AB...	DR...	DSA	CMV	HCV	HB...	Prev...	Type	ST...
6		OS	Surname:	First name:		2	1	HI	A	1	0	+	ND	ND	A1	KI	L	
6		OS	Surname:	First name:		14	3	HI	A	3	0	+	-	-		KI	L	
7		OS	Surname:	First name:		13	1	NI	A	2	0	+	-	-		KI		
7		OS	Surname:	First name:		1	1	NI	A	2	0	+	-	-		KI		

STAMP & LAMP

19. Calculated combined PRA and transplantability

A donor pool, based on 2000 recently HLA typed deceased donors registered in Scandiatransplant, has been made. The pool forms the basis of the following calculations.

19.1 Calculated combined PRA

The calculated PRA is based on the antibody summary and is updated automatically when list of identified antibodies is changed. Antibodies that are no longer clinical relevant and set as acceptable () are not included in the calculation.

This feature is accessible from two places:

1. From the 'STAMP Aux' tab

The screenshot shows the 'Waiting list information' form with the 'STAMP Aux' tab selected. The form contains fields for generic data, specific data, infection serology, STAMP/LAMP, STAMP QC, urgency history, and termination. The 'STAMP Aux' tab is highlighted with a red box. Below the tabs, the 'Antibody Summary' is displayed, followed by the 'Own HLA' field. At the bottom, the 'Calculated Combined PRA' is shown as 100%.

Waiting list information

Generic data

Scandia Number: Surname: Date of entry: 16-Feb-2012 Date of first urgency: 05-Mar-2012

Waiting list type: KI: Kidney Urgency: NT: Temporarily not Treatment center: AE: Rigshospitalet

Transplant center: CP: København Immunization: I: Immunized Date of last change of Immunization: 17-Mar-2015

STAMP Sign Up: Y: Yes STAMP Status: A: Active

Specific data Infection serology STAMP/LAMP **STAMP Aux** STAMP QC Urgency History Termination

Antibody Summary: A1,11,2,23,24,25,3,31,32,33,36,68,69,74,80; B13,18,27,35,37,38,39,41,42,45,46,48,49,50,51,52,53,54,55,56,57,58,59,60,61,62,63,64,65,67,7,71,72,75,76,77,78,8,81,82; Cw15,17,18,2,5,6; DQ6,8,9; DR10,103,12,13,14,15,16,17,18,4,7,8,9;

Own HLA: A26,29;B27,44;Cw1;Bw*w4;DR1,11;DQ5,7

Calculated Combined PRA: 100 %

2. From the menu 'All recipient', make a query on the specific patient and enter the antibody screen test tab.

The screenshot shows the 'Recipient information' form with the 'Antibody Screen Test' tab selected. The form contains fields for recipient information, basic info, clinical data, address/phone, waiting list, HLA typing, acceptable antibodies, previous mismatches, and death. The 'Antibody Screen Test' tab is highlighted with a red box. Below the tabs, the 'Antibody Summary' is displayed, followed by the 'Calculated combined PRA' field, which is highlighted with a red box and shows 95%. Below this, there is a table with columns for Date of sample, PRA Class I, PRA Class II, and Identified Antibodies.

Recipient information

Scandia Number: Nationality: SF: Finland Date of Birth: Person Number: Sex: F: Female

Surname: First Name: Transplantation History: (0)KI; LI; PA; IT; HE; LU; Survival Status: ALIVE

Waiting list status: N: Notified Waiting list type: KI: Kidney Urgency: T: Transplantable

First regist.: OPS\$SIVA 14-Feb-2014 Latest regist.: OPS\$PIIAR 18-May-2015

Basic info Clinical data Address/Phone Waiting List HLA Typing **Antibody Screen Test** Acceptable Antibodies Previous Mismatches Death

Antibody Summary: A2,29,3,31,33,68,69,74; B45,73,76,82; DQ4,5,6; DR12,8;

Calculated combined PRA: 95 % Immunization: HI: Highly immunized

Add new

Date of sample	PRA Class I	PRA Class II	Identified Antibodies
07-May-2015	90	88	
05-Feb-2015	87	88	A2,29,3,31,33,68,69,74; B45,73,76,82; DQ4...
06-Nov-2014	87	88	
07-Aug-2014	86	88	
08-May-2014	87	88	
06-Feb-2014	64	64	

19.2 Estimated transplantability score

The estimated transplantability scores are based on the latest antibody screen test result where HLA specificities have been defined. HLA-antigens to which the patients has no antibodies against are regarded as acceptable mismatches.

Based on split level HLA typing it gives you the percentage of donors in the pool which are ABO identical or compatible and have HLA split level antigens that are acceptable to the recipient (recipient HLA + Acceptable mismatches)

Recipient information Info Back Save Reset Print

Scandia Number: Nationality: N: Norway Sex: F: Female

Date of Birth: Person Number: ()

Surname: Surname: First Name: First name:

Transplantation History: (0)KI; LI; PA; IT; HE; LU; CO;

Recipient Status: ALIVE; on STAMP; on LAMP

Waiting list status: N: Notified Waiting list type: KI: Kidney Urgency: T: Transplantable Treatm. center: Haukeland

First regist.: 08-Oct-2020 Latest regist.: 18-Nov-2020

Basic info Clinical data Address/Phone HLA Typing **Antibody Screen Test** Fusion Acceptable Antibodies Previous Mismatches Death

Antibody Summary (Serological/serological equivalent): A:2,24,33,34,68,69 B:7,8,18,27,37,38,39,41,42,46,54,55,56,59,60,63,64,65,67,73,75,81,82 Cw:1,4,5,6,7,8,9,10,12,14,15,16,17,18 DQ:2 DR:7,9 DRB3/4/5:3*02

Calculated combined PRA: 100 % Immunization: HI: Highly immunized

Estimated Transplantability score

Compatible ABO: 0.00 % Identical ABO: 0.00 %

19.3 Transplantability score

The transplantability scores are based on split level HLA typing on the patient and defined acceptable mismatches. It gives you the percentage of donors which are ABO identical or compatible and have HLA split level antigens that are acceptable to the recipient (recipient HLA + Acceptable mismatches)

Specific data Infection **LAMP** LAMP QC **STAMP** STAMP log STAMP Aux STAMP QC Urgency History Termination

Determination Method: LUMI

Date of acceptance: 18-Nov-2020 Status: A: Active Sign up: Y: Yes

Acceptable mismatches

HLA-A: 1,11,23,25,26,29,30,31,36,43,66,74,80

HLA-B: 13,35,44,45,47,48,49,50,52,53,57,58,61,62,71,72,76,77,78

HLA-Cw:

HLA-DR: 3,8,10,11,12,13,14,15,16,17,18,103

HLA-DQ: 4,6,7,9

HLA-DP: 0101,0201,0301,0402,0501,0901,1001,1101,1301,1401,1501,1701,1801,1901,2001,2301,2801

HLA-DRB3/4/5: 3*01,3*03,5*01,5*02

HLA-DQA: 02,04,05,06

HLA-DPA: 02,03,04

Comments:

First Registr.: NAPEROS 09-Oct-2020 Last Change.: IDW 18-Nov-2020

Calculated transplantability score based on defined acceptable mismatches

Compatible ABO: 0.00 % Identical ABO: 0.00 % Normal match: 0.00 % Date of Calc: 08-Feb-2021

19.3 Normal match

'Normal match' is based on the patient HLA type and a 'normal' broad level A, B and DR match. It gives you the percentage of donors which are ABO identical and have no mismatches on HLA broad level A, B and DR with the recipient, similar to a priority 2 kidney exchange obligation.